

{書類名} 図面

{図1}

Fig. 1A

(a)


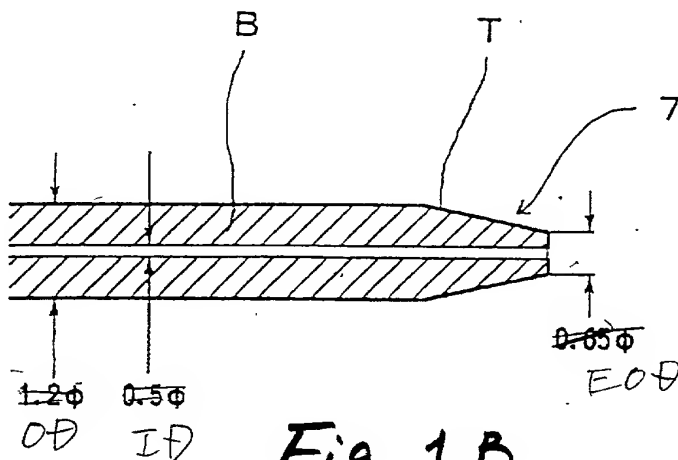


Fig. 1B

(b)

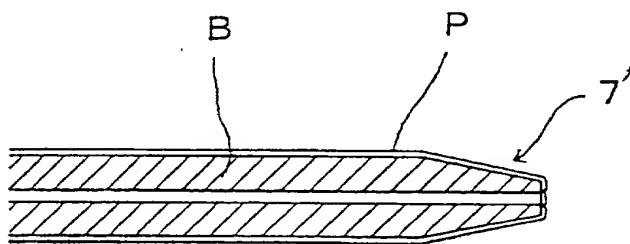


~~【図2】~~

Fig. 2A

(a)

VIAL No. = 20

Injection amount
注入量: 2

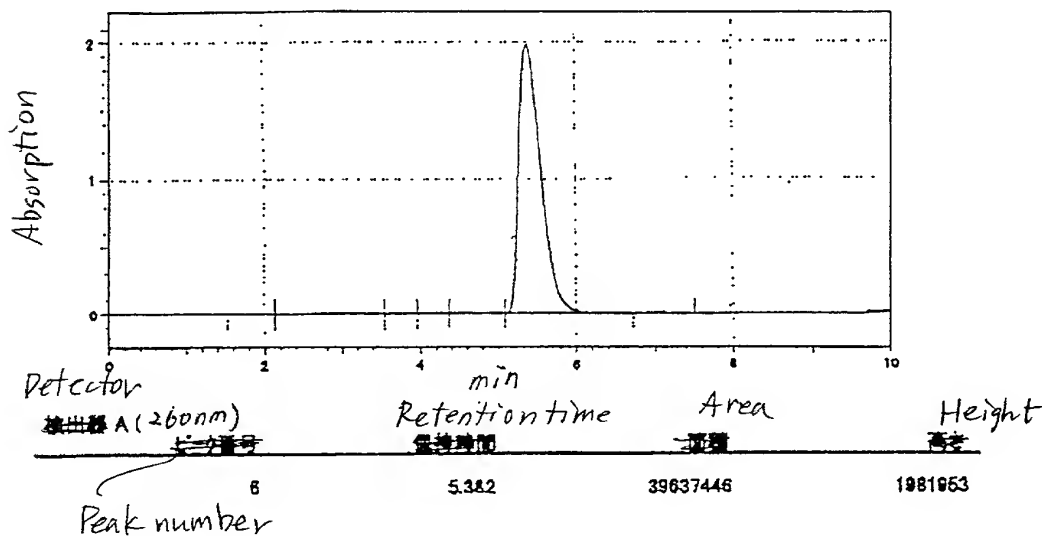


~~(b)~~

VIAL No. = 70

Injection amount
注入量: 2

Fig. 2B

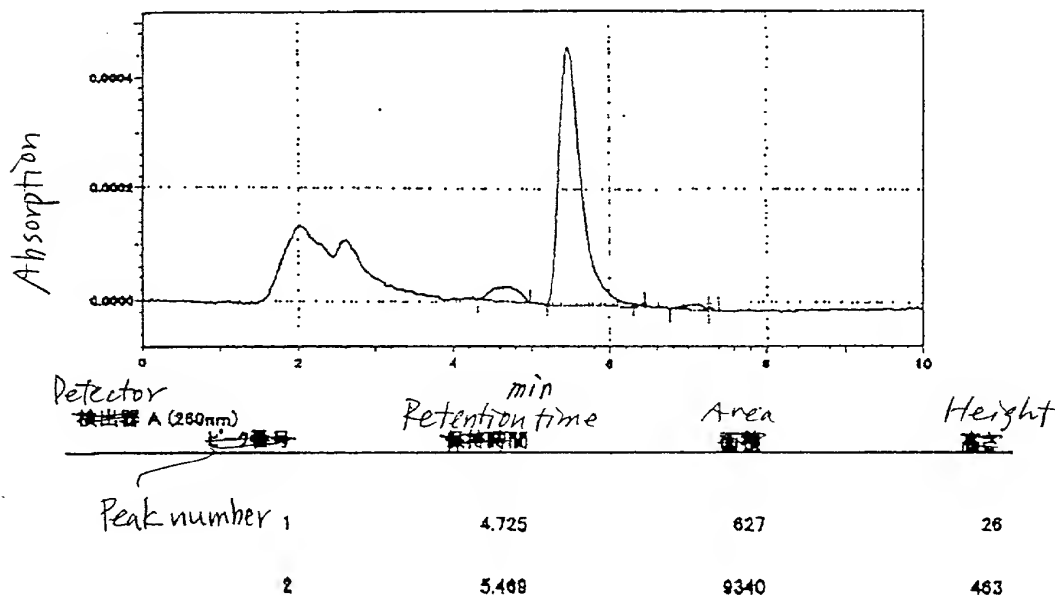

~~Fig. 3~~


Fig. 3A

~~(a)~~

VIAL No. = 10

注入量: 2

Injection amount

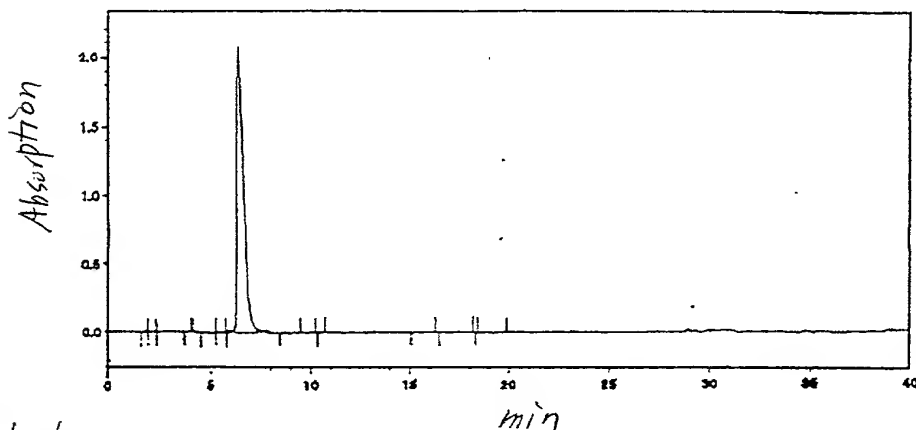

Detector

検出器 B (260nm)

Retention time

保持時間

6.525

Area

面積

48126387

Height

高さ

2067405


~~(b)~~

Fig. 3B

VIAL No. = 40

注入量: 2

Injection amount

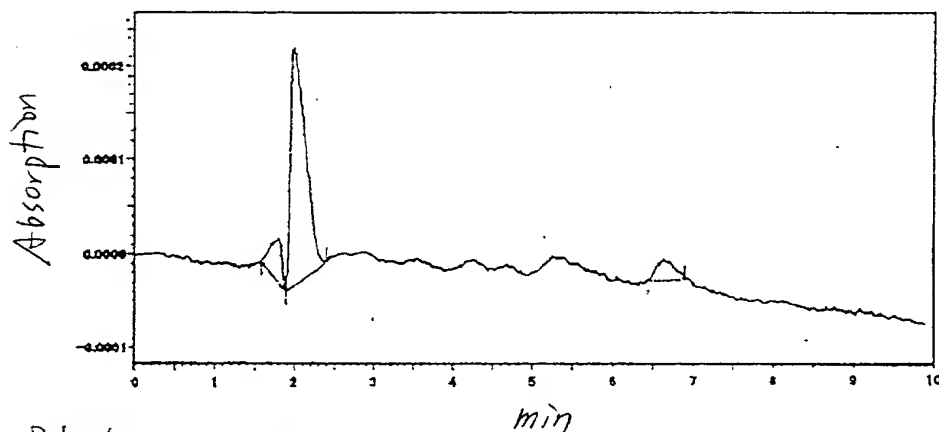

Detector

検出器 B (260nm)

Retention time

保持時間

6.653

Area

面積

321

Height

高さ

22

20040929001

~~【图4】~~